

1/4

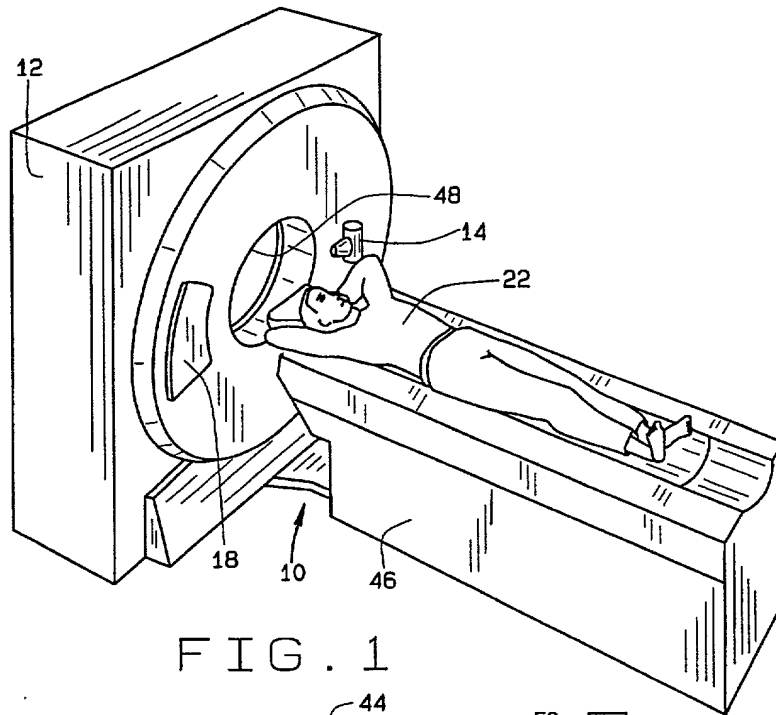


FIG. 1

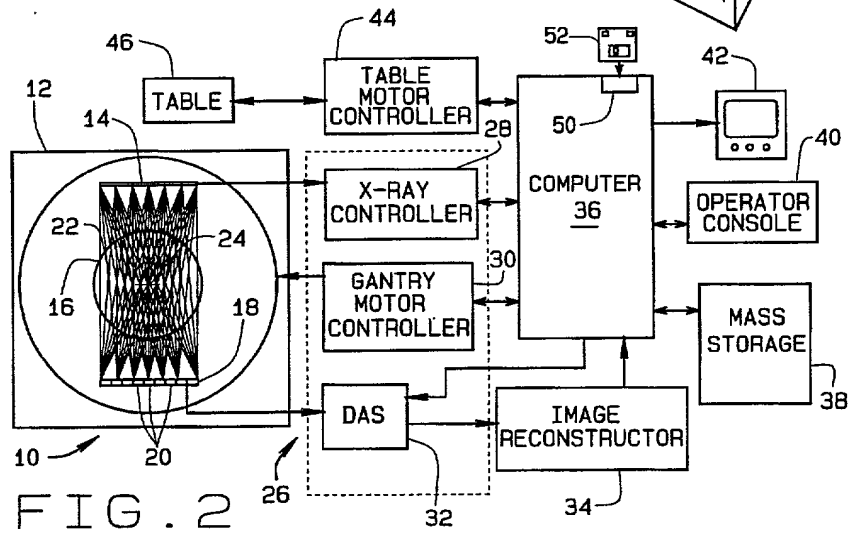


FIG. 2

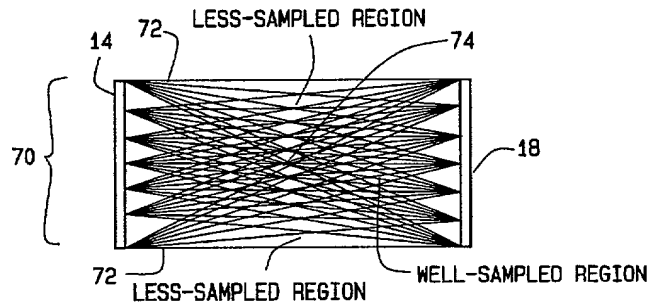


ILLUSTRATION OF INHOMOGENEOUS SAMPLING PATTERN

FIG. 3

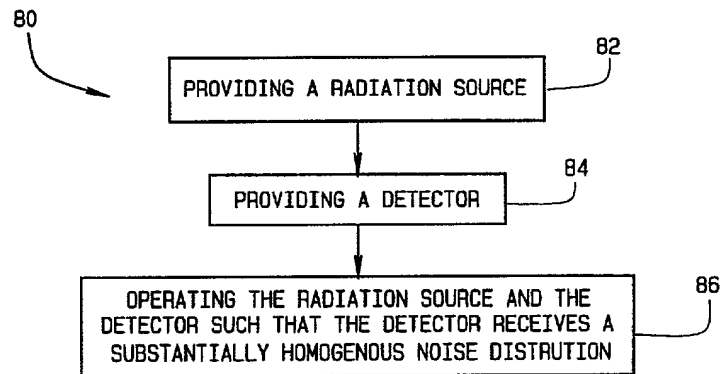


FIG. 4

3/4

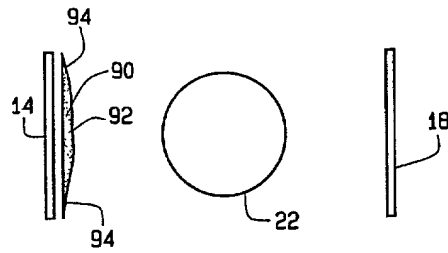


ILLUSTRATION OF THE PRE-PATIENT FILTER TO MODIFY THE X-RAY FLUX

FIG. 5

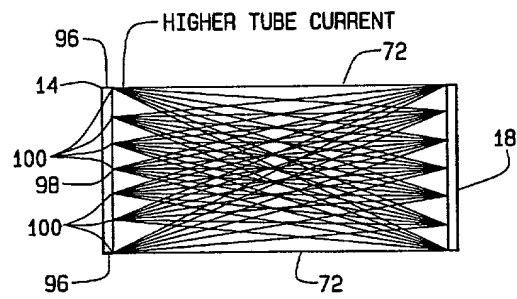


ILLUSTRATION OF TUBE CURRENT MODULATION APPROACH

FIG. 6

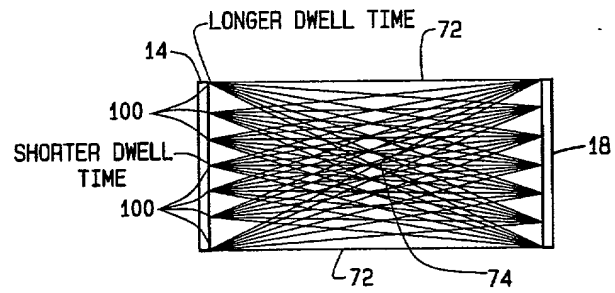


ILLUSTRATION OF DWELL TIME MODULATION APPROACH

FIG. 7

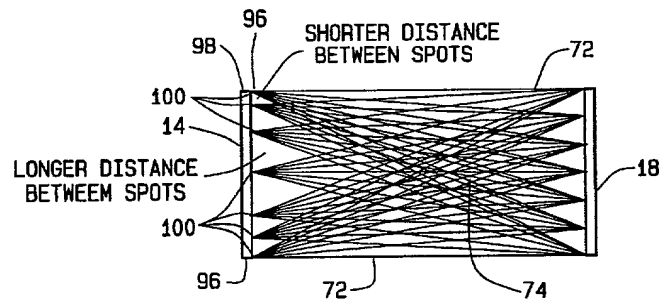


ILLUSTRATION OF UNEVENLY PACED X-RAY SPOTS

FIG. 8